


sgmTM


medical monitoring.

BRAIN

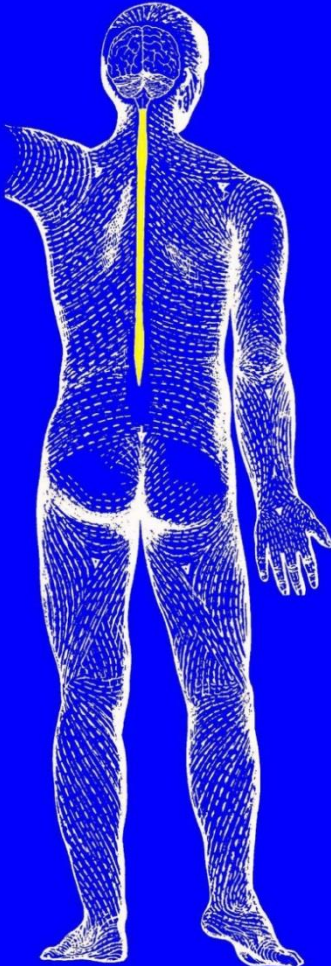

From

M
O
T
O
R



To
MUSCLES



spinal cord

To

S
E
N
S
O
R
Y



From
SKIN
MUSCLES
JOINTS

Cortexstim


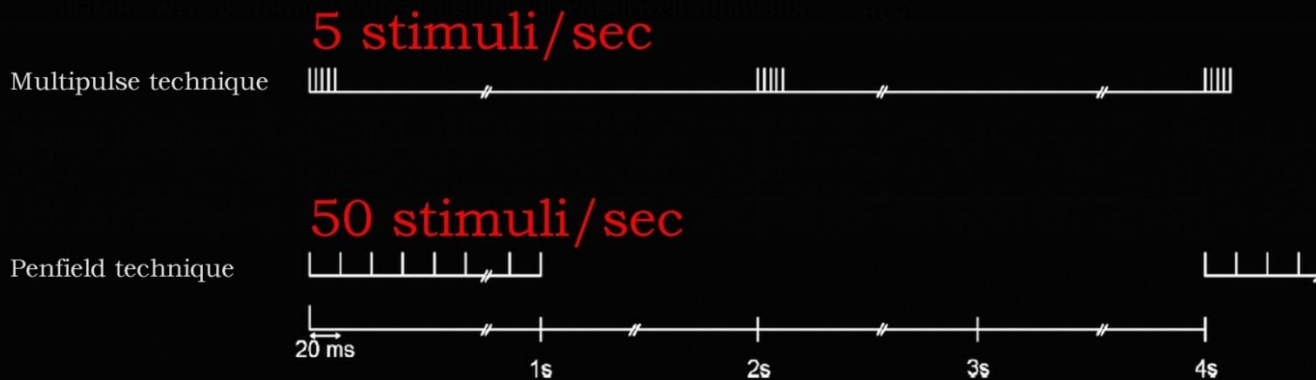


Fig. 1. Schematic drawing of the multipulse stimulation and the 50-Hz stimulation techniques. The individual pulse width is 0.5 ms. For the multipulse stimulation technique, the interstimulus interval was 4 ms, the repetition rate was 0.5 Hz. For the 50-Hz stimulation technique, the interstimulus interval was 20 ms. The total pulse stimulus duration was 1 s and repeated every 4 s.

Cortexstim u praksi

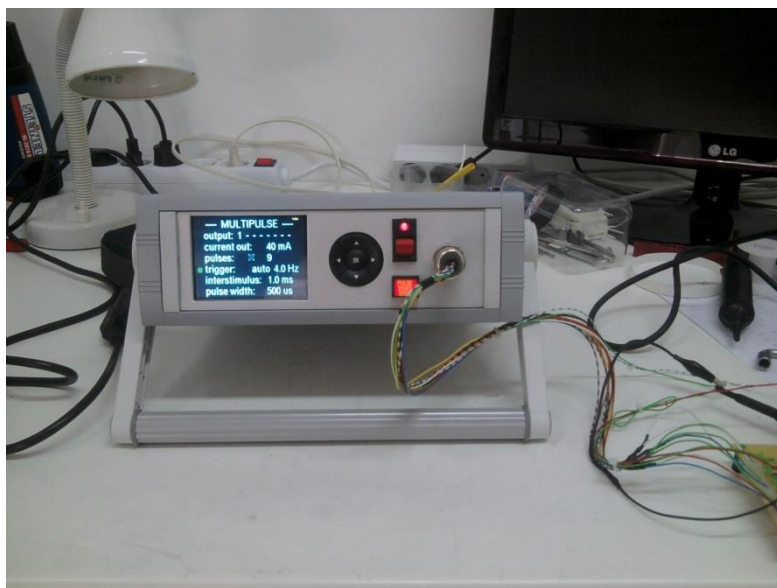

Budući cilj SGM-a

- Proširenje postojeće linije proizvoda SGM-a s ciljem razvoja tehnologije koja bi pružila realnu sliku stanja pacijenta za vrijeme operacijskog zahvata

